



For use with LightCycler1.0/2.0 Instrument

**1. Intended Use**

New Influenza A virus (H1N1) real time RT-PCR kit is used for the detection of new reassortment Influenza A virus (H1N1) by using real time PCR systems.

2. Principle of Real-Time RT-PCR

RT-PCR (Reverse Transcription-Polymerase Chain Reaction) is a technique in which an RNA strand is "reverses" transcribed into its DNA complement, followed by amplification of the resulting DNA using a polymerase chain reaction (PCR). RT-PCR can be used to examine gene expression level in cells and tissues, clone the specific gene of cDNA sequences and test RNA viruses. One Step RT-PCR Kit adopts one tube system. Because operator doesn't need to open the lid during the reaction process, this user-friendly improved version avoids cross contamination.

3. Product Description

Influenza A virus subtype H1N1 (A/H1N1), is a subtype of influenza A virus. It is the most common cause of influenza (flu) in humans. Some strains of H1N1 are endemic in humans, including the strain(s) responsible for the 1918 flu pandemic which killed 50–100 million people worldwide. Less virulent H1N1 strains still exist in the wild today, worldwide, causing a small fraction of all influenza-like illness and a large fraction of all seasonal influenza. In March and April 2009, hundreds of laboratory-confirmed infections and a number of deaths were caused by an outbreak of a new strain of H1N1. The new Influenza A virus real time RT-PCR kit contains a specific ready-to-use system for the detection of the new Influenza A virus (H1N1) using RT-PCR in the real-time PCR system. The primer and probe is designed for specifically detect new influenza virus (H1N1) with new reassortment genome. The reaction is done in one step real time RT-PCR. The first step is a reverse transcription (RT), during which the virus RNA is transcribed into cDNA. Afterwards, a thermostable DNA polymerase is used to amplify the specific gene fragments by means of PCR (polymerase chain reaction). Fluorescence is emitted and measured by the real time systems' optical unit during the PCR. The detection of amplified virus DNA fragment is performed in fluorimeter channel 530nm with the fluorescent quencher BHQ1. An external positive control is supplied which allow the determination of the gene load.

Internal control is available in the kit. It can be used for monitoring the yield of the nucleic acid extraction and whether there existing inhibition in the sample or not.

4. Kit Contents

Ref.	Type of reagent	Presentation	25rxns
1	New H1N1 Super Mix	1 vial, 350µl	
2	RT-PCR Enzyme Mix	1 vial, 28µl	
3	Molecular Grade Water	1 vial, 400µl	
4	New H1N1 Positive Control	1 vial, 30µl	
5	Internal Control	1 vial, 30µl	

Analysis sensitivity: 1×10⁴ copies/ml.

Note: Analysis sensitivity depends on the sample volume, elution volume, nucleic acid extraction methods and other factors. If you use the RNA extraction kits recommended, the analysis sensitivity is the same as it declares. However, when the sample volume is dozens or even hundreds of times greater than elution volume by some concentrating method, it can be much higher.

5. Storage

- All reagents should be stored at -20°C. Storage at +4°C is not recommended.
- All reagents can be used until the expiration date indicated on the kit label.
- Repeated thawing and freezing (> 3x) should be avoided, as this may reduce the sensitivity of the assay.
- Cool all reagents during the working steps.
- Super Mix should be stored in the dark.

6. Additionally Required Materials and Devices

- Biological cabinet
- Real time PCR system
- Real time PCR reaction tubes/plates
- Pipets (0.5 µl – 1000 µl)
- Sterile microtubes
- Biohazard waste container
- Desktop microcentrifuge for "ependorf" type tubes (RCF max. 16,000 x g)
- Tube racks
- Vortex mixer
- RNA extraction kit
- Cryo-container
- Sterile filter tips for micro pipets
- Disposable gloves, powderless
- Refrigerator and freezer

7. Warnings and Precaution

- Carefully read this instruction before starting the procedure.
- For in vitro diagnostic use only.
- This assay needs to be carried out by skilled personnel.
- Clinical samples should be regarded as potentially infectious materials and should be prepared in a laminar flow hood.
- This assay needs to be run according to Good Laboratory Practice.
- Do not use the kit after its expiration date.
- Avoid repeated thawing and freezing of the reagents, this may reduce the sensitivity of the test.
- Once the reagents have been thawed, vortex and centrifuge briefly the tubes before use.
- Prepare quickly the Reaction mix on ice or in the cooling block.
- Set up two separate working areas: 1) Isolation of the RNA/ DNA and 2) Amplification/ detection of amplification products.
- Pipets, vials and other working materials should not circulate among working units.
- Use always sterile pipette tips with filters.
- Wear separate coats and gloves in each area.
- Do not pipette by mouth. Do not eat, drink, smoke in laboratory.
- Avoid aerosols

8. Sample Collection, Storage and transport

- Collected samples in sterile tubes;
- Specimens can be extracted immediately or frozen at -20°C to -80°C.
- Transportation of clinical specimens must comply with local regulations for the transport of etiologic agents

9. Procedure**9.1 RNA-Extraction****9.1.1 Type of specimens**

A variety of specimens are suitable for the diagnosis of virus infections of the upper respiratory tract:

◆ Nasal swab	◆ Nasopharyngeal aspirate
◆ Nasopharyngeal swab	◆ Throat swab

In addition to swabs from the upper respiratory tract, invasive procedures can be performed for the diagnosis of virus infections of the lower respiratory tract where clinically indicated:

◆ Transtracheal aspirate	◆ Lung biopsy
◆ Bronchoalveolar lavage	◆ Post-mortem lung or tracheal tissue

Specimens for the laboratory diagnosis of avian influenza A should be collected in the following order of priority:

◆ Nasopharyngeal aspirate	◆ Convalescent serum
◆ Acute serum	

9.1.3 RNA extraction kits

Different brand RNA extraction kits are available. You may use your own extraction systems or the commercial kit based on the yield. For the RNA extraction, please comply with the manufacturer's instructions. The recommended Extraction kit is as follows:

Nucleic Acid Isolation Kit	Cat. Number	Manufacturer
RNA Isolation Kit	ME-0001	ZJ Biotech
QIAamp Viral RNA Mini extraction Kit (50)	52904	QIAGEN

9.2 Internal Control


It is necessary to add internal control (IC) in the reaction mix. Internal Control (IC) allows the user to determine and control the possibility of PCR inhibition.

Add the internal control (IC) 1µl/rxn and the result will be shown in the 560nm.

9.3 RT-PCR Protocol**1) Preparation of positive control and negative control**

It is necessary to dilute the positive control and internal control supplied in the kit by 10 times with molecular grade water before detection, and close the tube immediately then vortex for 10 seconds.

2) The Master Mix volume for each reaction should be pipetted as follows:

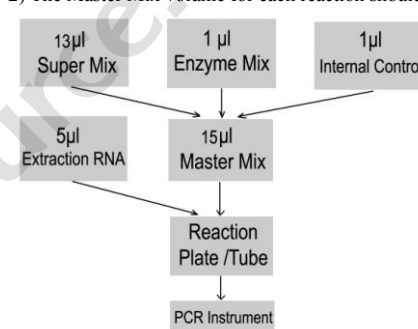

Attention: PCR system without 560nm channel (e.g. LightCycler1.0) can be treated with 1µl Molecular Grade Water instead of 1µl Internal Control.

3) The volumes of Super Mix and Enzyme Mix per reaction multiply with the number of reaction, which includes the number of controls, standards, and sample prepared. Molecular Grade Water is used as the negative control. For reasons of unprecise pipetting, always add an extra virtual sample. Mix

completely then spin down briefly in a centrifuge.

- Pipet 15µl Master Mix with micropipets of sterile filter tips to each of the Real time PCR reaction plate/tubes. Separately add 5µl RNA sample supernatant or positive and negative controls to different reaction plate/tubes. Immediately close the plate/tubes to avoid contamination.
- Spin down briefly in order to collect the Master Mix in the bottom of the reaction tubes.
- Perform the following protocol in the instrument:

45°C for 10min	1cycle	Selection of fluorescence channels
95°C for 15min	1cycle	
95°C for 5sec, 60°C for 30sec (Fluorescence measured at 60°C)	45cycles	
		530nm Target Nucleic Acid
		560nm IC

10. Threshold setting: Choose **Arithmetic** as back ground and **none** as Noise Band method, then adjust the Noise band just above the maximum level of molecular grade water, and adjust the threshold just under the minimum of the positive control.

11. Quality control: Negative control, positive control, and internal control must be performed correctly, otherwise the sample results is invalid.

Control	Channel	Crossing point value	
		530nm	560nm
Molecular Grade Water		Blank	25~35
Positive Control(qualitative assay)		≤35	—

12. Data Analysis and Interpretation : The following sample results are possible:

	Crossing point value		Result Analysis
	530nm	560nm	
1#	Blank	25~35	Below the detection limit or negative
2#	≤43	—	Positive; New Influenza A virus H1 subtype's genome bears strong resemblance to the genome of strain A/California/04/2009. If the results are obtained, it is likely that a new reassortment of the New Influenza A virus has emerged.
3#	43~45	25~35	Re-test; If it is still 38~40, report as 1#
4#	Blank	Blank	PCR Inhibition; No diagnosis can be concluded.

For further questions or problems, please contact our technical support



For use with ABI Prism®7000/7300/7500/7900/Step One Plus; iCycler iQ™4/iQ™5; Smart Cycler II; Bio-Rad CFX 96; Rotor Gene™ 6000; Mx3000P/3005P; MJ-Option2/Chromo4; LightCycler®480 Instrument



1. Intended Use

New Influenza A virus (H1N1) real time RT-PCR kit is used for the detection of new reassortment Influenza A virus (H1N1) by using real time PCR systems.

2. Principle of Real-Time RT-PCR

RT-PCR (Reverse Transcription-Polymerase Chain Reaction) is a technique in which an RNA strand is "reversed" transcribed into its DNA complement, followed by amplification of the resulting DNA using a polymerase chain reaction (PCR). RT-PCR can be used to examine gene expression level in cells and tissues, clone the specific gene of cDNA sequences and test RNA viruses. One Step RT-PCR Kit adopts one tube system. Because operator doesn't need to open the lid during the reaction process, this user-friendly improved version avoids cross contamination.

3. Product Description

Influenza A virus subtype H1N1 (A/H1N1), is a subtype of influenza A virus. It is the most common cause of influenza (flu) in humans. Some strains of H1N1 are endemic in humans, including the strain(s) responsible for the 1918 flu pandemic which killed 50–100 million people worldwide. Less virulent H1N1 strains still exist in the wild today, worldwide, causing a small fraction of all influenza-like illness and a large fraction of all seasonal influenza. In March and April 2009, hundreds of laboratory-confirmed infections and a number of deaths were caused by an outbreak of a new strain of H1N1. The new Influenza A virus real time RT-PCR kit contains a specific ready-to-use system for the detection of the new Influenza A virus (H1N1) using RT-PCR in the real-time PCR system. The primer and probe is designed for specifically detect new influenza virus (H1N1) with new reassortment genome. The reaction is done in one step real time RT-PCR. The first step is a reverse transcription (RT), during which the virus RNA is transcribed into cDNA. Afterwards, a thermostable DNA polymerase is used to amplify the specific gene fragments by means of PCR (polymerase chain reaction). Fluorescence is emitted and measured by the real time systems' optical unit during the PCR. The detection of amplified virus DNA fragment is performed in fluorimeter channel FAM with the fluorescent quencher BHQ1. An external positive control is supplied which allow the determination of the gene load. Internal control is available in the kit. It can be used for monitoring the yield of the nucleic acid extraction and whether there existing inhibition in the sample or not.

4. Kit Contents

Ref.	Type of reagent	Presentation	25rxns
1	New H1N1 Super Mix	1 vial, 480µl	
2	RT-PCR Enzyme Mix	1 vial, 28µl	
3	Molecular Grade Water	1 vial, 400µl	
4	New H1N1 Positive Control	1 vial, 30µl	
5	Internal Control	1 vial, 30µl	

Analysis sensitivity: 5×10³ copies/ml.

Note: Analysis sensitivity depends on the sample volume, elution volume, nucleic acid extraction methods and other factors. If you use the RNA extraction kits recommended, the analysis sensitivity is the same as it declares. However, when the sample volume is dozens or even hundreds of times greater than elution volume by some concentrating method, it can be much.

5. Storage

- All reagents should be stored at -20°C. Storage at +4°C is not recommended.
- All reagents can be used until the expiration date indicated on the kit label.
- Repeated thawing and freezing (> 3x) should be avoided, as this may reduce the sensitivity of the assay.

- Cool all reagents during the working steps.

- Super Mix should be stored in the dark.

6. Additionally Required Materials and Devices

- Biological cabinet
- Real time PCR system
- Real time PCR reaction tubes/plates
- Pipets (0.5 µl – 1000 µl)
- Sterile microtubes
- Biohazard waste container
- Desktop microcentrifuge for "eppendorf" type tubes (RCF max. 16,000 x g)
- Tube racks
- Vortex mixer
- RNA extraction kit
- Cryo-container
- Sterile filter tips for micro pipets
- Disposable gloves, powderless
- Refrigerator and freezer

7. Warnings and Precaution

- Carefully read this instruction before starting the procedure.
- For in vitro diagnostic use only.
- This assay needs to be carried out by skilled personnel.
- Clinical samples should be regarded as potentially infectious materials and should be prepared in a laminar flow hood.
- This assay needs to be run according to Good Laboratory Practice.
- Do not use the kit after its expiration date.
- Avoid repeated thawing and freezing of the reagents, this may reduce the sensitivity of the test.
- Once the reagents have been thawed, vortex and centrifuge briefly the tubes before use.
- Prepare quickly the Reaction mix on ice or in the cooling block.
- Set up two separate working areas: 1) Isolation of the RNA/ DNA and 2) Amplification/ detection of amplification products.
- Pipets, vials and other working materials should not circulate among working units.
- Use always sterile pipette tips with filters.
- Wear separate coats and gloves in each area.
- Do not pipette by mouth. Do not eat, drink, smoke in laboratory.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC OR THERAPEUTIC PROCEDURES.

- Avoid aerosols

8. Sample Collection, Storage and transport

- Collected samples in sterile tubes;
- Specimens can be extracted immediately or frozen at -20°C to -80°C.
- Transportation of clinical specimens must comply with local regulations for the transport of etiologic agents

9. Procedure

9.1 RNA-Extraction

9.1.1 Type of specimens

A variety of specimens are suitable for the diagnosis of virus infections of the upper respiratory tract:

◆ Nasal swab	◆ Nasopharyngeal aspirate
◆ Nasopharyngeal swab	◆ Throat swab

In addition to swabs from the upper respiratory tract, invasive procedures can be performed for the diagnosis of virus infections of the lower respiratory tract where clinically indicated:

◆ Transtracheal aspirate	◆ Lung biopsy
◆ Bronchoalveolar lavage	◆ Post-mortem lung or tracheal tissue

Specimens for the laboratory diagnosis of avian influenza A should be collected in the following order of priority:

◆ Nasopharyngeal aspirate	◆ Convalescent serum
◆ Acute serum	

9.1.2 RNA extraction kits

Different brand RNA extraction kits are available. You may use your own extraction systems or the commercial kit based on the yield. For the RNA extraction, please comply with the manufacturer's instructions. The recommended Extraction kit is as follows:

Nucleic Acid Isolation Kit	Cat. Number	Manufacturer
RNA Isolation Kit	ME-0010/ME-0012	ZJ Biotech
QIAamp Viral RNA Mini extraction Kit(50)	52904	QIAGEN

Respiratory specimens should be collected and transported in virus transport media.

Virus transport medium

(A) Virus transportation medium use in collecting throat and nasal swabs

1) Add 10g veal infusion broth and 2g bovine albumin fraction V to sterile distilled water (to 200ml). 2) Add 0.8ml gentamicin sulfate solution(50mg/ml) and 3.2ml amphotericin B(250µg/ml). 3) Sterilize by filtration.

B) Nasal wash medium: Sterile saline(0.85% NaCl)


9.2 Internal Control

It is necessary to add internal control (IC) in the reaction mix. Internal Control (IC) allows the user to determine and control the possibility of PCR inhibition.

Add the internal control (IC) 1µl/rxn and the result will be shown in the HEX/VIC/JOE.

9.3 RT-PCR Protocol

The Master Mix volume for each reaction should be pipetted as follows:

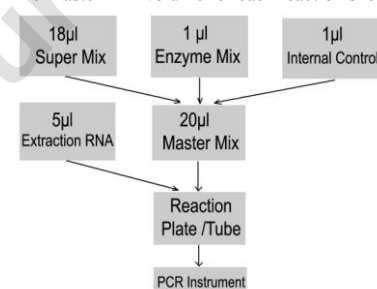

1) The volumes of Super Mix and Enzyme Mix per reaction multiply with the number of reaction, which includes the number of controls, standards, and sample prepared. Molecular Grade Water is used as the negative control. For reasons of unprecise pipetting, always add an extra virtual sample. Mix completely then spin down briefly in a centrifuge.

2) Pipet 20µl Master Mix with micropipets of sterile filter tips to each of the Real time PCR reaction plate/tubes. Separately add 5µl RNA sample supernatant or positive and negative controls to different reaction plate/tubes. Immediately close the plate/tubes to avoid contamination.

3) Spin down briefly in order to collect the Master Mix in the bottom of the reaction tubes.

4) Perform the following protocol in the instrument:

45°C for 10min	1cycle
95°C for 15min	1cycle
95°C for 15sec, 60°C for 1min	45cycles
(Fluorescence measured at 60°C)	

Selection of fluorescence channels	
FAM	Target Nucleic Acid
HEX/VIC/JOE	IC

5) ⚠ If you use ABI Prism® system, please choose "none" as passive reference and quencher.

10. Threshold setting: just above the maximum level of molecular grade water.

11. Quality control: Negative control, positive control, and internal control must be performed correctly, otherwise the sample results is invalid.

Channel		Ct value	
Control		FAM	HEX/VIC/JOE
Molecular Grade Water		UNDET	25~35
Positive Control(qualitative assay)		≤35	—

12. Data Analysis and Interpretation : The following sample results are possible:

	Ct value		Result Analysis
	FAM	HEX/VIC/JOE	
1#	UNDET	25~35	Below the detection limit or negative
2#	≤43	—	Positive; New Influenza A virus H1 subtype's genome bears strong resemblance to the genome of strain A/California/04/2009. If the results are obtained, it is likely that a new reassortment of the New Influenza A virus has emerged.
3#	43~45	25~35	Re-test; If it is still 38~40, report as 1#
4#	UNDET	UNDET	PCR Inhibition; No diagnosis can be concluded.

For further questions or problems, please contact our technical support